

TENMARS

TM-104 Sound Level Meter User's Manual



HB2TM1040000

Contents:

1	Introduction	1
2	Accessories.....	1
3	Safety.....	1
4	Meter description.....	2
5	Operation	3
5.1	Disable auto power off.....	4
5.2	Maximum and Minimum hold.....	4
5.3	Data hold.....	4
5.4	94dB Calibration.....	5
6	General Specifications	6
7	Electrical Specifications:.....	7
8	Maintenance	8
9	Battery Replacement.....	8
10	Disposal	9

TENMARS



1 Introduction

This sound level meter is a digital noise meter auto-shifting function that can be applied to the measurements for both environmental noise and mechanical noise.

2 Accessories


- 1 Meter
- 1 User's Manual
- 1 9V battery
- 1 Carrying case
- 1 Windscreen

3 Safety

	Caution! Please refer to this manual. Improper use may damage the meter and its components.
	Compliance with European Directive

- Do not operate in environments with flammable gas or humid environments.
- Do not place the meter in locations with high temperature, humid, or exposed to direct sunlight.
- Operating altitude: 2000 meters below sea level.
- Operation environment: Indoor use; contamination level class 2.
- EMC: EN61326-1:CISPR 11:Group 1, Class B
- ✧ **Class B** – Equipment is suitable for use in domestic establishments and outside facilities.
- ✧ **Group 1** – RF energy generated is needed for internal functioning.


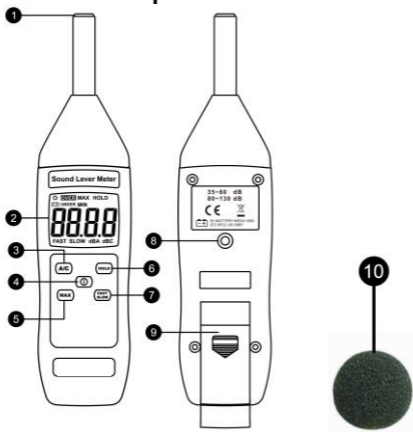


4 Meter description



1. Microphone.
2. LCD display
3. A /C weighting select button.
4. Power button
5. Maximum and Minimum hold button
6. Data hold button.
7. Time weighting select button.
8. Tripod nut.
9. Battery cover.
10. Windscreen.

TENMARS


5 Operation

- Press  to turn on or turn off.
- Please select dBA for the measurement of acoustic noise, dBC for the measurement and analysis of mechanical noise, wherein click  to switch the modes.
- Select "FAST" to read the instantaneous noise level, "SLOW" to read the average noise level, wherein click  to switch the modes.
- Press  to capture the maximum or minimum noise level and lock the readings.
- When measuring noise with the sound level meter by hand, keep the distance between the microphone and the sound source by about 1~1.5 meters.



Warning


Wind blowing across the microphone would bring additional extraneous noise. Once using the instrument in the presence of wind with speed higher than 10m/s, it must mount the windscreen to prevent the undesirable signals.

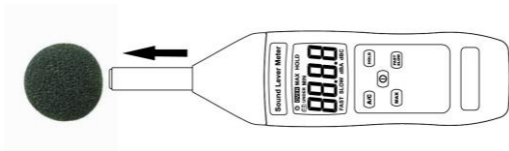





TENMARS

5.1 Disable auto power off


The meter is preset to shutdown automatically after 15-minute inactivity.


When powering on, press  for 2 seconds to disable the auto shutdown function which can be set to disable or enable as needed.

5.2 Maximum and Minimum hold

Click  for less than 1 second to view the maximum and minimum values cyclically, while pressing  and  for switching frequency weighting and time weighting. Press and hold  for more than 1 second to quit the function.

5.3 Data hold


Click  to enable or disable the data hold function.

When "HOLD" is activated, all buttons will be disabled, except for .

TENMARS

5.4 94dB Calibration

- Carefully plug the microphone head into the 1/2 inch hole of the standard audio source (94dB, @1KHz sine wave).
 - Turn on the power of the standard audio source (94dB, @1KHz sine wave).
 - Press and hold **(A/C)** + **(HOLD)** for more than 1 second and enter the 94dB correction function.
 - Press **(MAX)** for auto calibration.
 - Press **(A/C)** to select frequency weighting.
 - Use the **(HOLD)** / **(FAST SLOW)** to manually adjust the deviation value (± 3.5 dB).
 - Press **(1)** to quit the 94dB correction function.
- * Auto correction range is 90.5~97.5dB.
* The meter has been calibrated as ex-factory. The calibration period is recommended as 1 year.



6 General Specifications


- 4 digital LCD.
- Frequency weighting: dBA, dBC
- Time weighting: FAST, SLOW
- Data hold.
- Autoranging.
- Auto power off(default 15 min)and disable auto power off.
- Maximum and Minimum hold
- Overloading “OVER” or “UNDER”.
- Low battery indication
- Battery: 9V (NEDA 1604 、 IEC 6F22 or JIS 006P)
- Battery life: About 50 hrs (alkaline Battery)
- Standby power consumption: 9uW
- Operating power consumption: 90mW
- Operation temperature and humidity:
5 to 40°C(41 to 104°F); < 80%RH
- Storage temperature and humidity:
-10°C to 60°C(14 to 140°F),< 70%RH
- Weight: about 200g(including battery)
- Dimension: 235(L) x 56(W) x 40(H)mm

7 Electrical Specifications:

Environmental conditions at 23°C ± 5°C


Sample rate	1 second
Standard applied	IEC 61672-1 class 2 IEC651 Type2 ANSI1.4 Type2
Microphone	1/2 inch Electret condenser microphone.
Dynamic Range	50 dB
Measuring range	35 ~ 130 dBA
	40 ~ 130 dBC
Frequency response	31.5 Hz ~ 8 KHz
Resolution	0.1 dB
Time weighting	FAST 125 ms ; SLOW 1s
Frequency weighting	A / C
Accuracy	±1.8 dB (reference SPL 94 dB @1KHZ)

8 Maintenance

1. When the When  symbol is displayed on the LCD, it means that there is insufficient power; please change the battery immediately in order to ensure its accuracy.
2. Do not place the meter in locations that have high temperature, humidity or that are exposed to direct sunlight.
3. Remember to turn off the power after usage; remove the battery if not used for a long period of time in order to prevent battery leakage and causing damages to internal components.
4. When the instrument failure, only by the authorized service provider or return the original repair.

9 Battery Replacement

1. Turn off the power.
2. Open the battery cover at the back of the meter, remove the batteries.
3. Please insert six new 9V batteries according to the polarities.
4. Put the battery cover back in place.



TENMARS

10 Disposal



Note: This symbol indicates that the meter and its accessories must be separated and processed properly.

TENMARS ELECTRONICS CO., LTD.
6F, NO.586 Ruiguang Rd, Neihu
Dist. Taipei City, Taiwan
E-mail: service@tenmars.com
<http://www.tenmars.com>